



Assessment of the Quality of Postero-anterior Chest Radiographs Seen in a North-west Nigerian Tertiary Hospital

**U. Abubakar^{1*}, A. Ibrahim¹, V. K. Nwodo², A. A. Sadiq¹, G. M. Akpaniwo¹,
A. Mohammed¹, D. Mohammed¹, I. I. Yusuf¹ and A. D. Gurama¹**

¹*Department of Radiography, Faculty of Clinical Sciences, College of Health Sciences, Usmanu Danfodiyo University, Sokoto, Nigeria.*

²*Department of Radiography and Radiological Sciences, Faculty of Health Sciences and Technology, College of Health Sciences, Nnamdi Azikiwe University, Nnewi Campus, Nigeria.*

Authors' contributions

This work was carried out in collaboration among all authors. Author UA designed the study, performed the statistical analysis, wrote the protocol and wrote the first draft of the manuscript. Authors AI and VKN managed the analyses of the study. Authors AAS, GMA, AM and DM managed the literature searches. All authors read and approved the final manuscript.

Article Information

DOI: 10.9734/JAMPS/2019/v21i130120

Editor(s):

(1) Dr. Amr Ahmed El-Arabey, Department of Pharmacology and Toxicology, Al-Azhar University, Egypt and University of Science and Technology of China (USTC), China.

Reviewers:

(1) A. Ayeshamariam, Khadir Mohideen College, India.
(2) Hadijat Oluseyi Kolade-Yunusa, University of Abuja, Nigeria.
(3) Umezurike Benedict Chidozie, Government House Clinic, Nigeria.
Complete Peer review History: <http://www.sdiarticle3.com/review-history/49869>

Original Research Article

**Received 24 April 2019
Accepted 06 July 2019
Published 10 July 2019**

ABSTRACT

Objectives: To determine the quality of chest radiographs of adult patients x-rayed at Usmanu Danfodiyo University Teaching Hospital (UDUTH) in accordance with Committee of European Commission (CEC) guidelines on quality criteria and to determine the most common factor that affects the radiographs.

Materials and Methods: The data was collected retrospectively from the hospital archives using a data capture sheet.

Results: A total of 266 radiographs were assessed and the age of patients whose radiographs participated in the study ranged from 20-80years. Also, a greater number of male patients

*Corresponding author: E-mail: umar.abubakar5@udusok.edu.ng;

147(55.3%) participated in the study than female patients 119(44.7%). Results from the study revealed that 194(72.93%) and 225(84.59%) radiographs had correct placement of patient details and anatomical marker respectively. Adequate inspiration was achieved in 223(83.83%) radiographs with presence of artifacts seen in only 17(6.39%) radiographs. Thrown-off scapulae out of lung fields was seen in 174(65.41%) radiographs while adequate penetration was demonstrated in 209(78.57%) radiographs. Fog was seen in 16(6.02%) radiographs and rotation was recorded in 86(32.33%) radiographs. Additionally, blurring and darkroom processing faults affected 9(3.38%) and 42(15.79%) radiographs respectively. The most common cause of poor quality chest radiographs was found to be inadequate collimation affecting 110(41.35%) radiographs.

Conclusion: In terms of overall quality, only about 41(15.41%) radiographs met all criteria for a standard chest radiograph according to committee of European commission.

Keywords: Postero-anterior; chest radiographs; quality; Nigeria.

1. INTRODUCTION

1.1 Background of the Study

Chest radiography is the most common examination used as one of the initial steps to diagnose pulmonary disease including respiratory infections [1]. Approximately 25% of all x-ray examinations performed accounts for Chest radiography [2]. Reports revealed that exposure to ionizing radiation increases the risks of some cancers at organ dose range of approximately 50–100 mSv [3,4]. The role of chest radiography has gained increased importance in trauma cases, routine check-ups, disease conditions and metastatic problems. The rationale behind this study is that many faulty diagnoses by chest radiography may be associated with inappropriate radiological techniques and application. The improvement of imaging quality of chest radiography benefits not only the patients infected by disease but also those suffering from various pulmonary diseases. In terms of detection and treatment of pulmonary diseases, poor imaging quality may be more harmful to patients than having the patients not diagnosed through x-ray procedures. Chest radiograph with poor image quality can cause misdiagnoses or require repeated examinations, wasting economic resources and exposing patients to unnecessary radiation. Conversely, providing high quality image of chest radiograph benefits anyone who will be examined by x-ray, and the precise control of these x-ray images is an important task for the radiographers.

Quality assurance (QA) refers to the planned and systematic activities implemented in a quality system so that quality requirements for a product or service will be fulfilled [5]. It is the systematic measurement comparison with a standard,

monitoring of processes and an associated feedback loop that confers error prevention. Quality assurance in chest radiography is a system designed to continuously improve the quality of chest radiographs at a health facility, and it can be achieved through organized efforts by all staff members involved in taking or reading the chest radiograph. It comprises quality control, quality assessment, and quality improvement [6]. Quality control includes all quality control efforts routinely performed by staff at each health facility such as regular maintenance or checking of x-ray equipment, accessory devices, chemicals and consumables.

2. MATERIALS AND METHODS

A retrospective descriptive study design was used for the study. A secondary data source was adopted which was recorded using data capture sheet. The data were obtained from the archives of Radiology department of Usmanu Danfodiyo University Teaching Hospital (UDUTH) and were selected based on convenience. The data were obtained by examining the patients' chest radiographs. Seven hundred and ninety four (794) radiographs of patients that underwent chest radiography from January 2017 to May 2018 at UDUTH were collected. The radiographs assessed were of examinations performed in the erect postero-anterior position and x-ray machine used for the examinations was GE MEDICAL SYSTEM (Model: MS-18S).

A convenient sampling technique was used for the study with Taro Yamane's formula used for sample size determination which was 266. Postero-anterior chest radiographs of adults were included [7]. All other projections of adult and paediatric cases were excluded. Data was collected via patients' chest radiographs and information like sex and age were recorded.

Standard criteria according to the committee of European commission was used to assess the radiographs [8].

Data was analysed using descriptive statistics mainly percentages and the data were presented using Tables, bar and pie charts.

3. RESULTS

A total of 266 chest radiographs were assessed out of which 147 were for male patients (55.3%) while 119 were for female patients (44.7%). This information is captured in Table 3.1.

Table 3.1. Gender distribution of patients

| Gender | Number(N) | Percentage (%) |
|--------|-----------|----------------|
| Male | 147 | 55.3 |
| Female | 119 | 44.7 |
| Total | 266 | 100 |

Age distribution of patients as shown in Table 3.2 revealed the age range of patients that participated in the study with age range of 20-35 having the highest participation with 107 radiographs (40.23%) while age range of 66-80 had the lowest participation with 12 radiographs (4.51%).

Table 3.3 shows the image criteria used in assessing the radiographs with number of radiographs in each criteria marked as 'Yes' for positive and 'No' for negative. It shows that anatomical coverage occurred more across all respondents with 243 radiographs demonstrating good anatomical coverage (91.35%) while presence of blurring occurred less with 9 radiographs, (3.38%). Fig. 3.1 is a bar chart showing the percentages of radiographs for each criteria with blue depicting 'Yes'(positive) and 'No' depicted by red colour.

The major causes of poor quality affecting all radiographs studied are shown in Table 3.4. Inadequate collimation was the highest among the major causes of poor quality affecting 110 radiographs (41.35%) while inadequate penetration was the lowest affecting 57 radiographs (21.43%).

Finally, information on criteria met by radiographs as a measure of quality are highlighted in Table 3.5. Only 41 radiographs representing 15.41% met all criteria according to European guidelines on quality of chest radiographs while the remaining 84.59% did not. This is demonstrated in Fig. 3.2.

Table 3.2. Age distribution of patients

| Age range | Number(N) | Percentages |
|-----------|-----------|-------------|
| 20-35 | 107 | 40.23 |
| 36-50 | 97 | 36.47 |
| 51-65 | 50 | 18.79 |
| 66-80 | 12 | 4.51 |
| Total | 266 | 100 |

4. DISCUSSION

This study has assessed the quality of postero-anterior chest radiographs using the radiographs of patients obtained from the archive of the department of diagnostic radiology, UDUTHS. The assessment was made with 12 criteria for assessing the quality of chest radiographs according to committee of European commission (CEC) guidelines [9].

The male patients appeared to be in larger number than female patients during the time of the study. All the chest radiographs used in this work consists of patients whose age ranges from 20 years to 80 years.

Findings from this study revealed that the major cause of poor quality radiographs was inadequate collimation which was seen in 41.35% of radiographs. This is in agreement with similar studies conducted by Okeji et al. [8]. The purpose of collimation is to protect the patient from unnecessary radiation by limiting the beam field to the anatomy of interest thereby reducing the volume of tissue irradiated. Poor collimation increases the radiation dose to the patients evoking possibility of stochastic effects of radiation. Poor collimation here can be attributed to radiographers not paying due attention to radiation protection probably to avoid repeats in case of cut-off. It could also be as a result of inexperience on the part of some of the interns in the department.

Another major cause of poor quality identified was inadequate throw-off of the scapulae seen in 92 radiographs (34.59%). This is in agreement with a study conducted by Okeji et al. (37.5%). It is important for the scapulae to be thrown-off the lungs field for a good quality chest radiograph to be achieved. It was found that the radiographers found it difficult to rotate the shoulders of sick elderly patients. Another cause of poor throw-off of the scapulae could be attributed to lack of proper instructions given to patients as well as patients shifting in between positioning and exposure. It could also be attributed to the nature of the patient particularly obese patients.

Table 3.3. Radiograph criteria

| Criteria | Yes (%) | No (%) | Total (%) |
|-----------------------------|------------|------------|-----------|
| Patient details | 194(72.93) | 72(27.07) | 266(100) |
| Anatomical marker | 225(84.59) | 41(15.41) | 266(100) |
| Anatomical coverage | 243(91.35) | 23(8.65) | 266(100) |
| Full inspiration | 223(83.83) | 43(16.17) | 266(100) |
| Presence of artifact | 17(6.39) | 249(93.61) | 266(100) |
| Scapulae out of lung fields | 174(65.41) | 92(34.59) | 266(100) |
| Adequate penetration | 209(78.57) | 57(21.43) | 266(100) |
| Fog | 16(6.02) | 250(93.98) | 266(100) |
| Rotation | 86(32.33) | 180(67.67) | 266(100) |
| Blurring | 9(3.38) | 257(96.62) | 266(100) |
| Adequate Collimation | 156(58.65) | 110(41.35) | 266(100) |
| Darkroom processing faults | 42(15.79) | 224(84.21) | 266(100) |




Fig. 3.1. Image criteria

Table 3.4. Major causes of poor quality radiographs

| Causes of poor quality | Frequency | Percentages (%) |
|-----------------------------|-----------|-----------------|
| Inadequate collimation | 110 | 41.35 |
| Scapulae out of lung fields | 92 | 34.59 |
| Rotation | 180 | 67.67 |
| No patient details | 72 | 27.07 |
| Inadequate penetration | 57 | 21.43 |

Rotation was another major factor that contributed to poor quality radiographs in this study which was noticed in 86 radiographs (32.3%). Similar finding was obtained in studies conducted by Okeji *et al* , Ugwuanyi et al. and Chand et al. who also reported rotation as a major cause of poor quality radiographs [8,10,11]. The medial ends of clavicle must be equidistant from the spinous process according to CEC guidelines for a radiograph to be devoid of rotation. Faults could be from improper positioning or improper instructions given to patients. Condition of the patient also predisposes to rotation as is the case in geriatric patients as well as very sick patients.

Table 3.5. Criteria met by radiographs

| Number of radiographs | Number of criteria met | Percentages |
|-----------------------|------------------------|-------------|
| 41 | 12 | 15.41 |
| 45 | 11 | 16.92 |
| 72 | 10 | 27.07 |
| 50 | 9 | 18.80 |
| 32 | 8 | 12.03 |
| 17 | 7 | 6.39 |
| 7 | 6 | 2.63 |
| 2 | 5 | 0.75 |
| Total | 266 | 100 |

Another major cause of poor quality obtained from the research was lack of patient details on 72 radiographs (27.07%) studied. This is contradictory to findings by Ugwuanyi *et al*. Improper identification can be attributed to radiographers and darkroom technician's negligence in ensuring correct placement of patient details on each radiograph processed. This could lead to mix-up and loss of patients' radiographs leading to misdiagnosis and to repeats thereby adding to patient dose respectively.

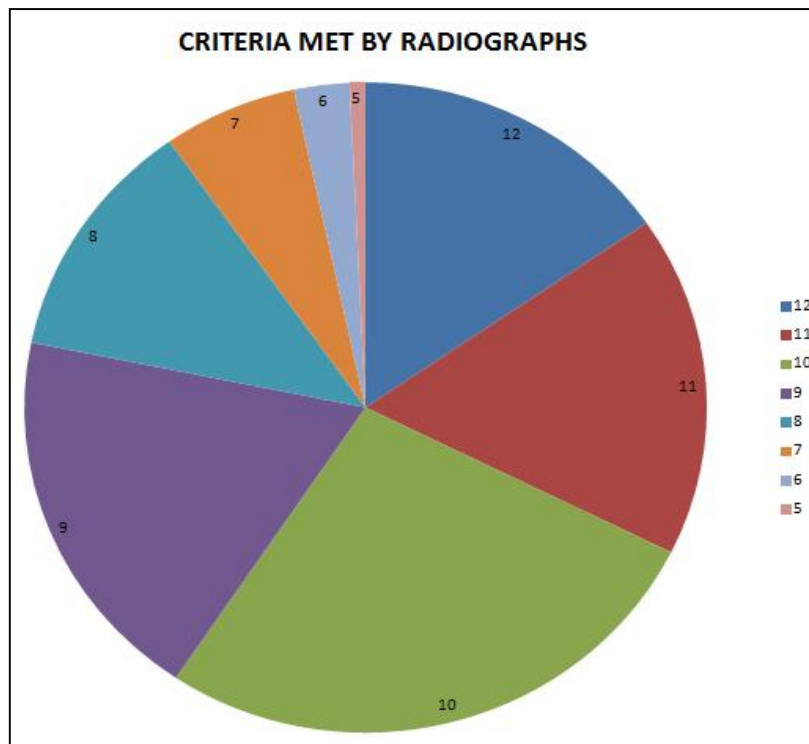


Fig. 3.2. Criteria met by radiographs

Also, inadequate penetration was observed in 21.43% of radiographs studied. This was consistent with findings by Ugwuanyi et al. (26.7%), Chand et al. (24%), and Okeji et al. (28%). The major cause of inadequate penetration is underexposure as demonstrated by ill-definition of lower intervertebral disc below 9th thoracic vertebra. This could result in the radiograph being repeated adding unnecessary radiation dose to the patient and incurring unnecessary cost to the department.

In terms of the overall quality of all the radiographs studied according to committee of European commission (CEC) recommendations, only 41(15.41%) radiographs met all the 12 criteria. Similar findings was obtained by Okeji et al.

Also, 45 (16.92%), 72(27.07%), 50(18.80%), 32(12.03%), 17(6.39%), 7(2.63%), and 2(0.75%) radiographs met 11, 10, 9, 8, 7, 6, and 5 criteria respectively meaning that about 84.59% radiographs did not meet all the recommended criteria. collimation and beam alignment quality assurance test should be carried out periodically to ensure light-beam alignment to the radiation field and hence radiation will not fall outside the area of interest after collimation by the radiographer [12].

5. CONCLUSION

The most common fault affecting the radiographs studied was inadequate collimation with majority of radiographs having either silver lining in less than 3 edges of the radiographs or excessive exposure of the abdomen indicating poor radiation protection. It can be deduced from this study that the skills of the radiographer as well as state of the equipment affects the quality of chest radiographs. It was found that in some instances due to economic considerations, chest radiographs that were sub-standard were accepted in the department. There should be efforts by radiographers to adhere to international standards as outlined in the European guidelines. This would avail the physicians of chest radiographs of good diagnostic quality, save costs incurred by the department and more importantly prevent unnecessary radiation to patients.

Conclusion is lengthy and contains unnecessary information. Kindly review.

European Commission-European guide- lines on quality criteria for diagnostic radiographic

images. Brussels, European Commission; 1996.

CONSENT

It is not applicable.

ETHICAL APPROVAL

It is not applicable.

COMPETING INTERESTS

Authors have declared that no competing interests exist.

REFERENCES

1. Eugene D, Robin N. Routine chest x-ray examinations. *Chest Journal*. 2010;90(2): 258-262.
2. International Commission on Radiation Units and Measurements. Image quality in chest radiography. ICRU Report 70, 2003. [ISBN: 1473-6691]
3. Boice JD Jr. The boice report no. 42, *Health Physics News*. 2015;152-154.
4. Matsumoto H, Tomita M, Otsuka K, Hatashita M. A new paradigm in radioadaptive response developing from microbeam research. *Journal of Radiation Research*. 2009;50:A67-A79.
5. Gloria M, Hani A. Quality assurance in radiology. *American journal of Roentgenology*. 2012;199(4):441-443.
6. Noha E. The concept of quality, quality assurance and quality enhancement. *Quality assurance in education*. 2015; 23(3):250-261.
7. Joseph EN. Sample size determination in qualitative and quantitative research; 2017. Available:<https://educacinfo.com/sample-size-determination-qualitative-quantitative-research/>. Accessed on 13th October 2018.
8. Okeji MC, Agwuna KK, Abubakar U, Izge IY, Animworie AU, Arogundade IO. Evaluation of diagnostic quality of chest radiographs seen in a Nigerian teaching hospital. *Journal of Advances in Medicine and Medical Research*. 2017;23(3):1-6.
9. European Commission-European guidelines on quality criteria for diagnostic radiographic images. Brussels, European Commission; 1996.
10. Ugwuanyi DC, Chiegwu H, Ngozika E. Evaluation of compliance with standard

- criteria for postero-anterior(PA) chest radiographs in parklane hospital Enugu. Journal of advances in medicine and medical research. 2018;23(3):1-6.
11. Chand RB, Thapa N, Paudal S, Pokharel GB, Joshi BR, Pant DK. Evaluation of image quality in chest radiographs. Journal of Institute of Medicine. 2013;35(1):50-52.
12. Okeji MC, Idigo FU, Anakwue AC, Nwogu UB, Meniru IO. Status of light beam diaphragm and its implication in radiation protection. World Applied Sciences Journal. 2016;34(7):975-978.

© 2019 Abubakar et al.; This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Peer-review history:

*The peer review history for this paper can be accessed here:
<http://www.sdiarticle3.com/review-history/49869>*